

**Volume determination of roundwood with individual method using automated device
accuracy report**
__ half of 20__

Recipients:

- (processing site)
- The Joint Advisory Council
- VMF LATVIA

1. Measurement method -


↳ **Tree species -**

↳ **Volume deviation +/- ... %** (rounded to one decimal place);

↳ **Standard deviation ... %** (rounded to one decimal place).

Number of control logs ... pieces.

1) VOLUME DEVIATION

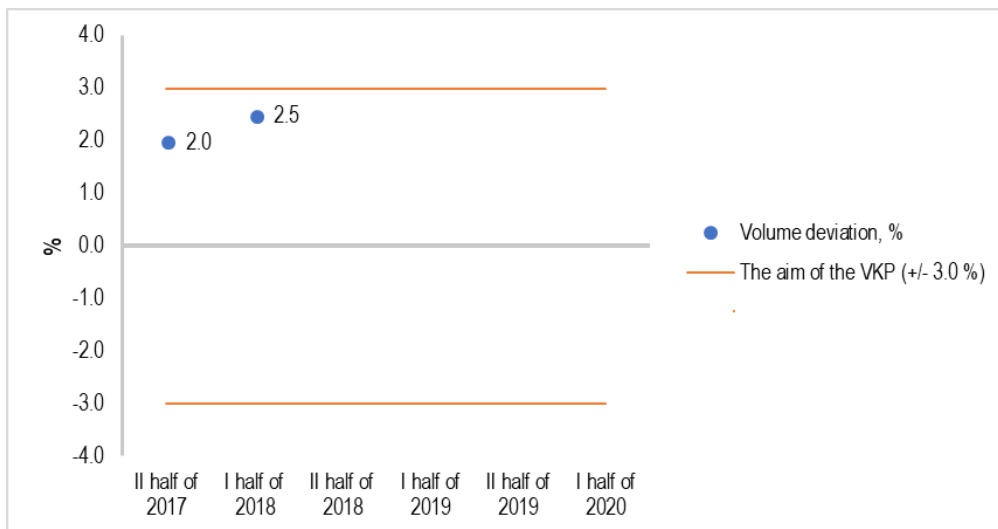

2) STANDARD DEVIATION

